


Software Version : 6.3.0.0445  
Sample Name : F134 S117301 WZ4002  
Instrument Name : Perkin Elmer LC  
Rack/Vial : 0/0  
Sample Amount : 1.000000  
Cycle : 1

Channel : A  
Operator : manager  
Dilution Factor : 1.000000

Result File : D:\YZR\F134 S117301 WZ4002.rst

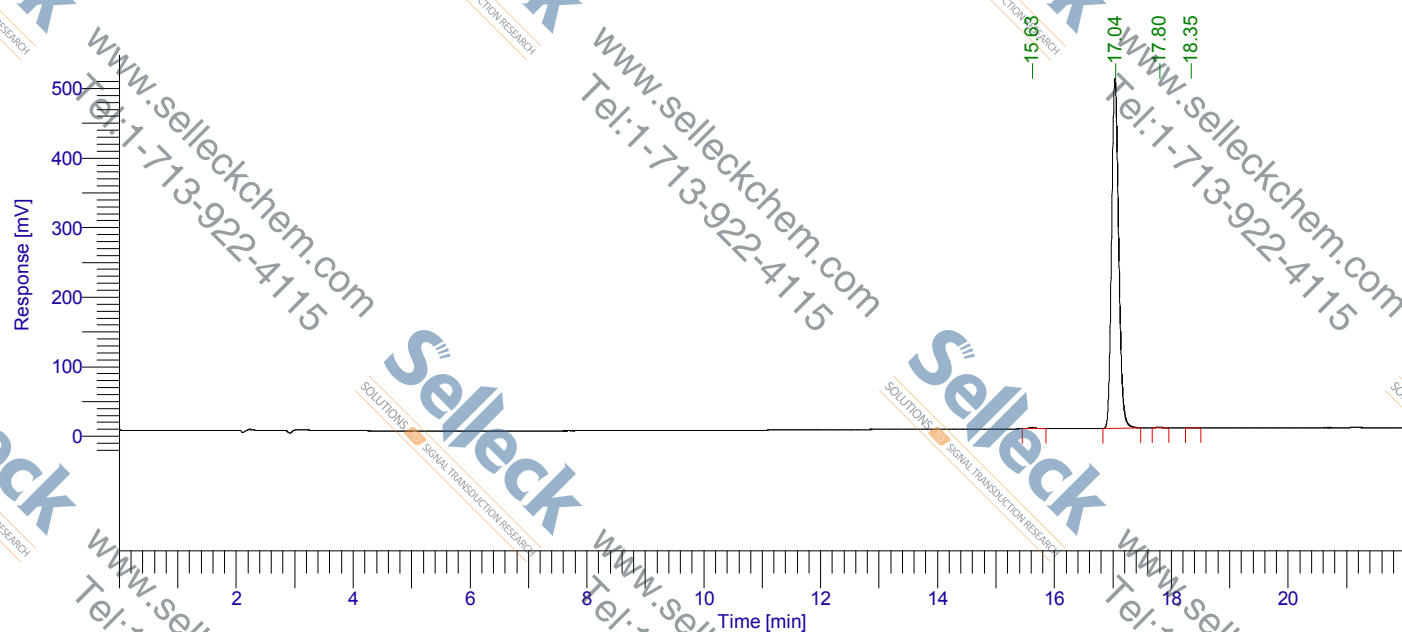

## HPLC REPORT

Peak #	Time [min]	Area [uV*sec]	Height [uV]	Area [%]	BL
1	15.627	15291.76	1768.73	0.357	MM
2	17.043	4256359.80	503069.74	99.312	MM
3	17.800	10159.62	1319.72	0.237	MM
4	18.347	4024.65	532.15	0.094	MM
		4285835.82	506690.35	1e+02	